




Comparison MeanSkin(M10 980127) Vs. MeanLatex100%Pwr(M10 980309)

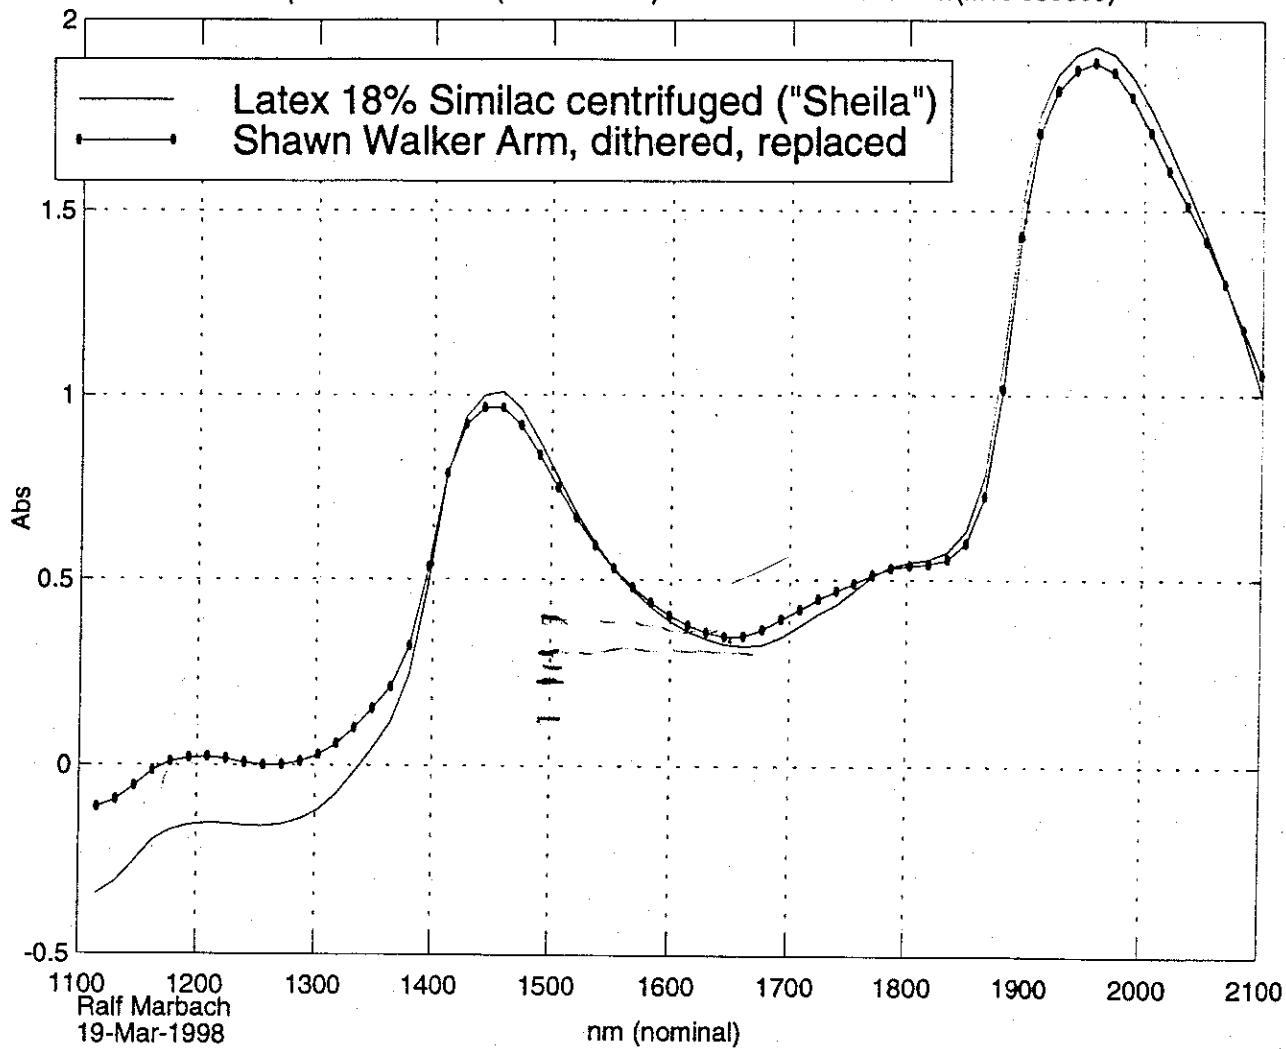


M20 12Feb98, Jerry's Cuvette Fixture

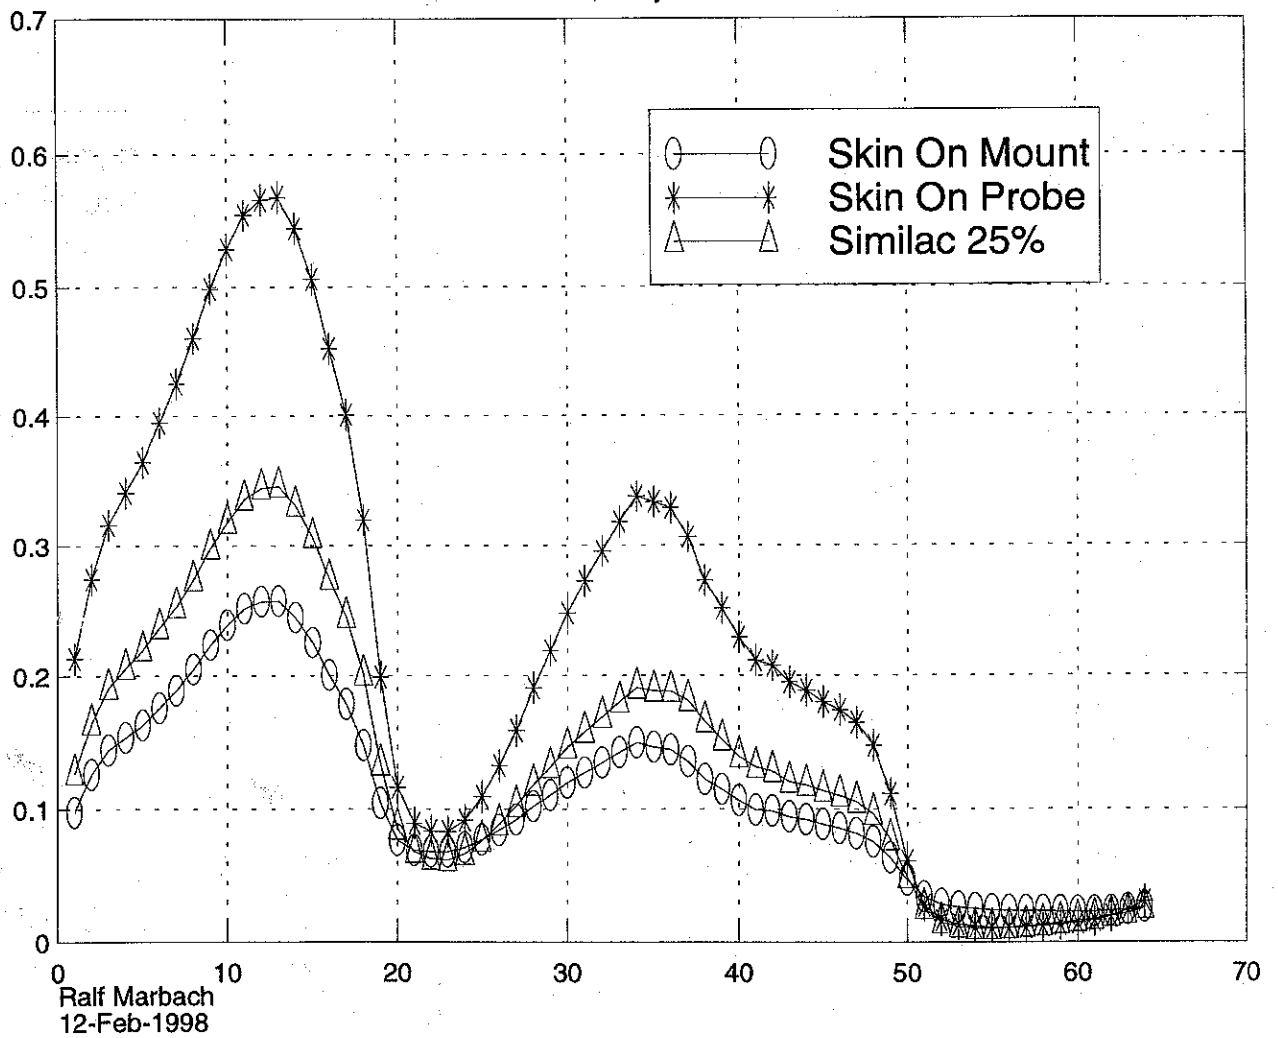

M20 12Feb98, Jerry's Cuvette Fixture, Offset corrected at #55

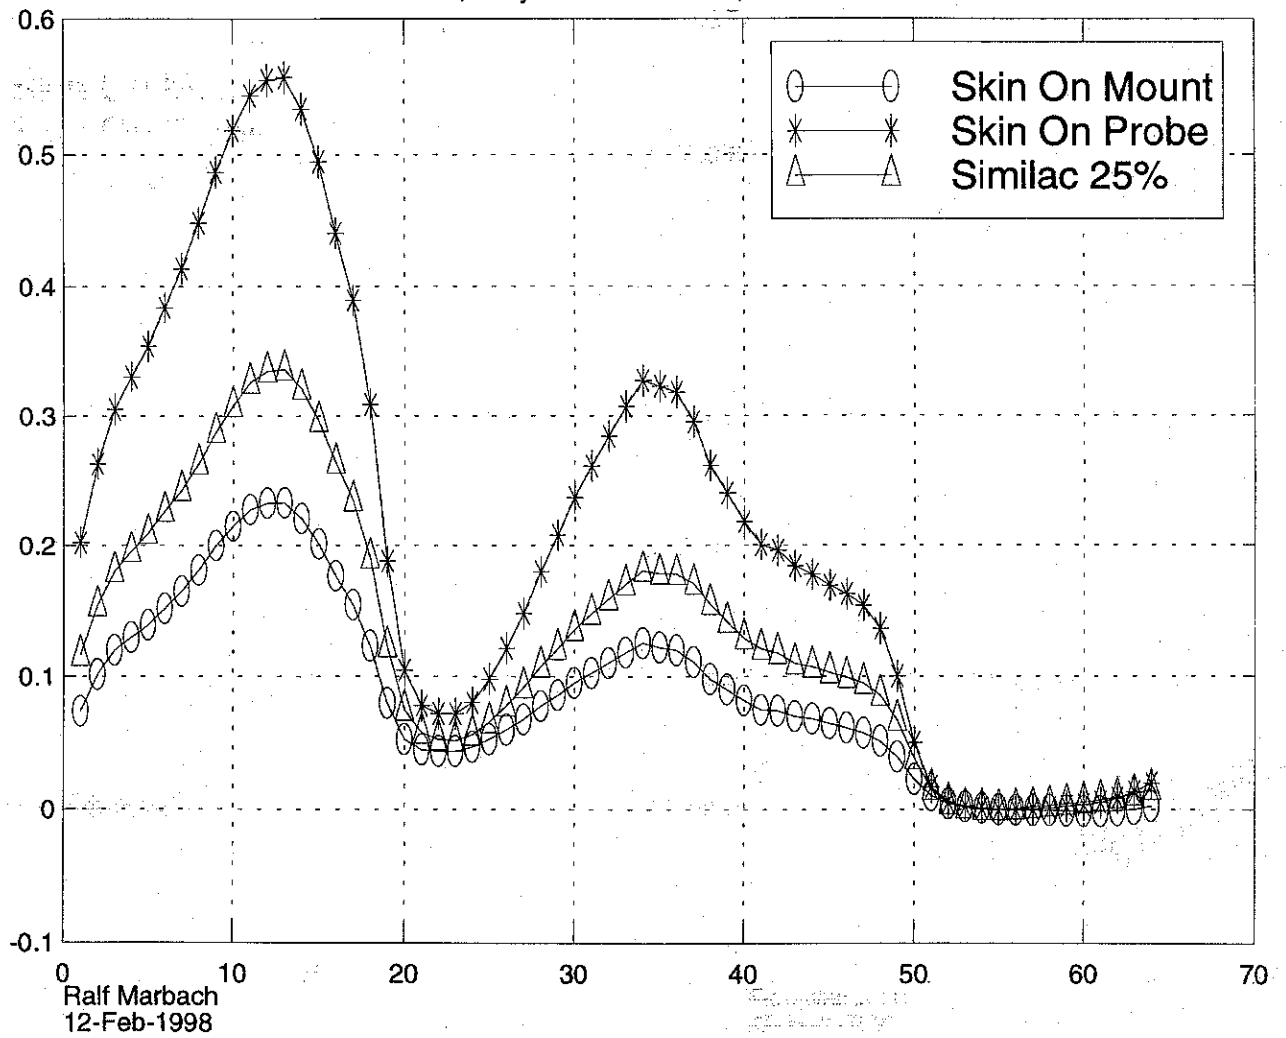

Skin on Probe / Skin on Mount

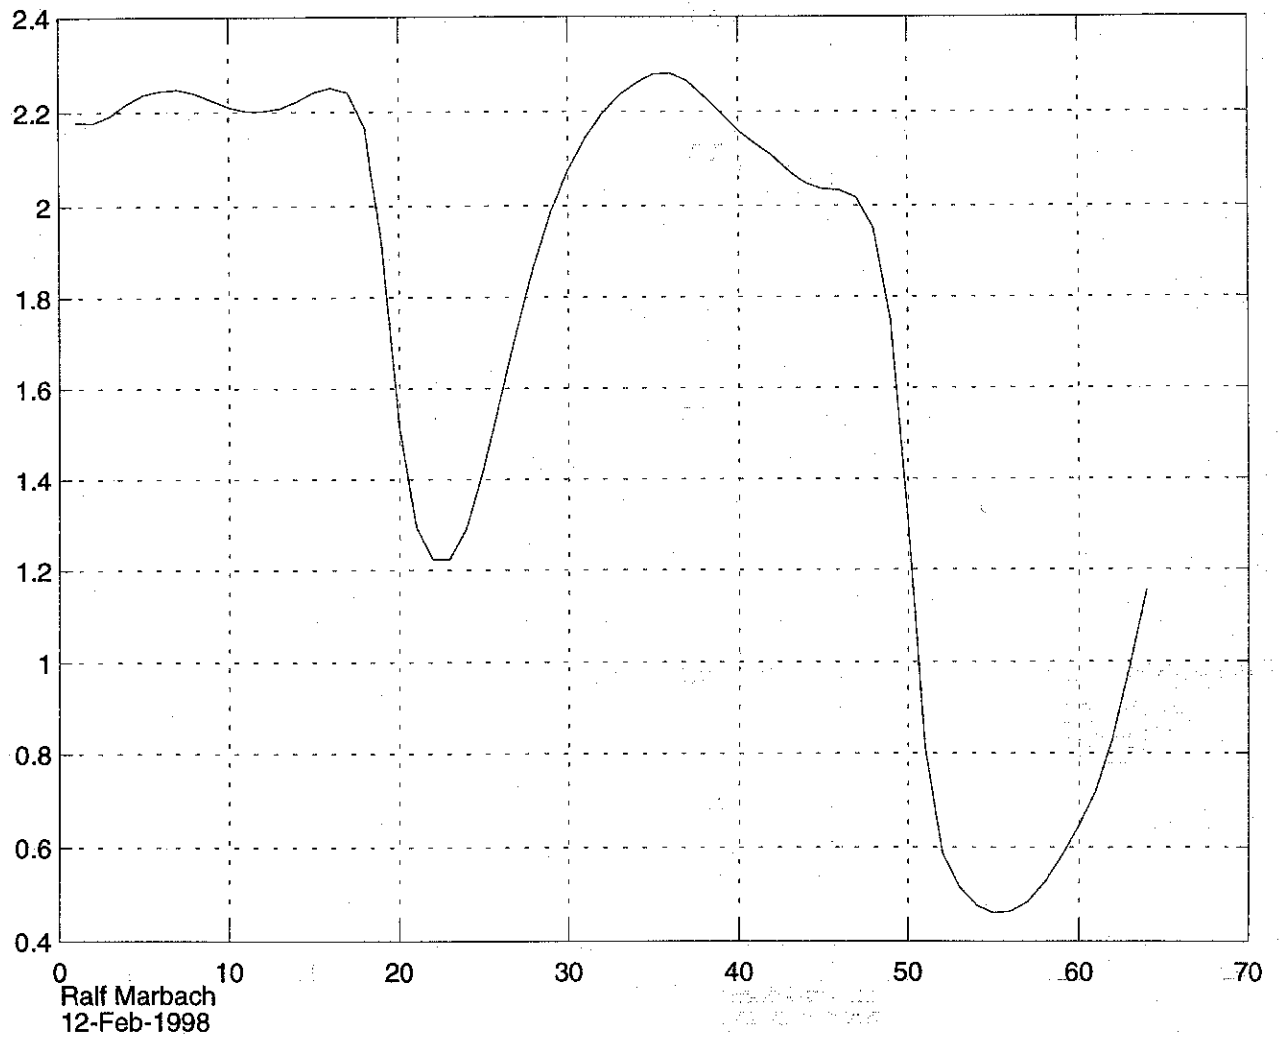

Skin on Probe / Similac

